


FIG. 1

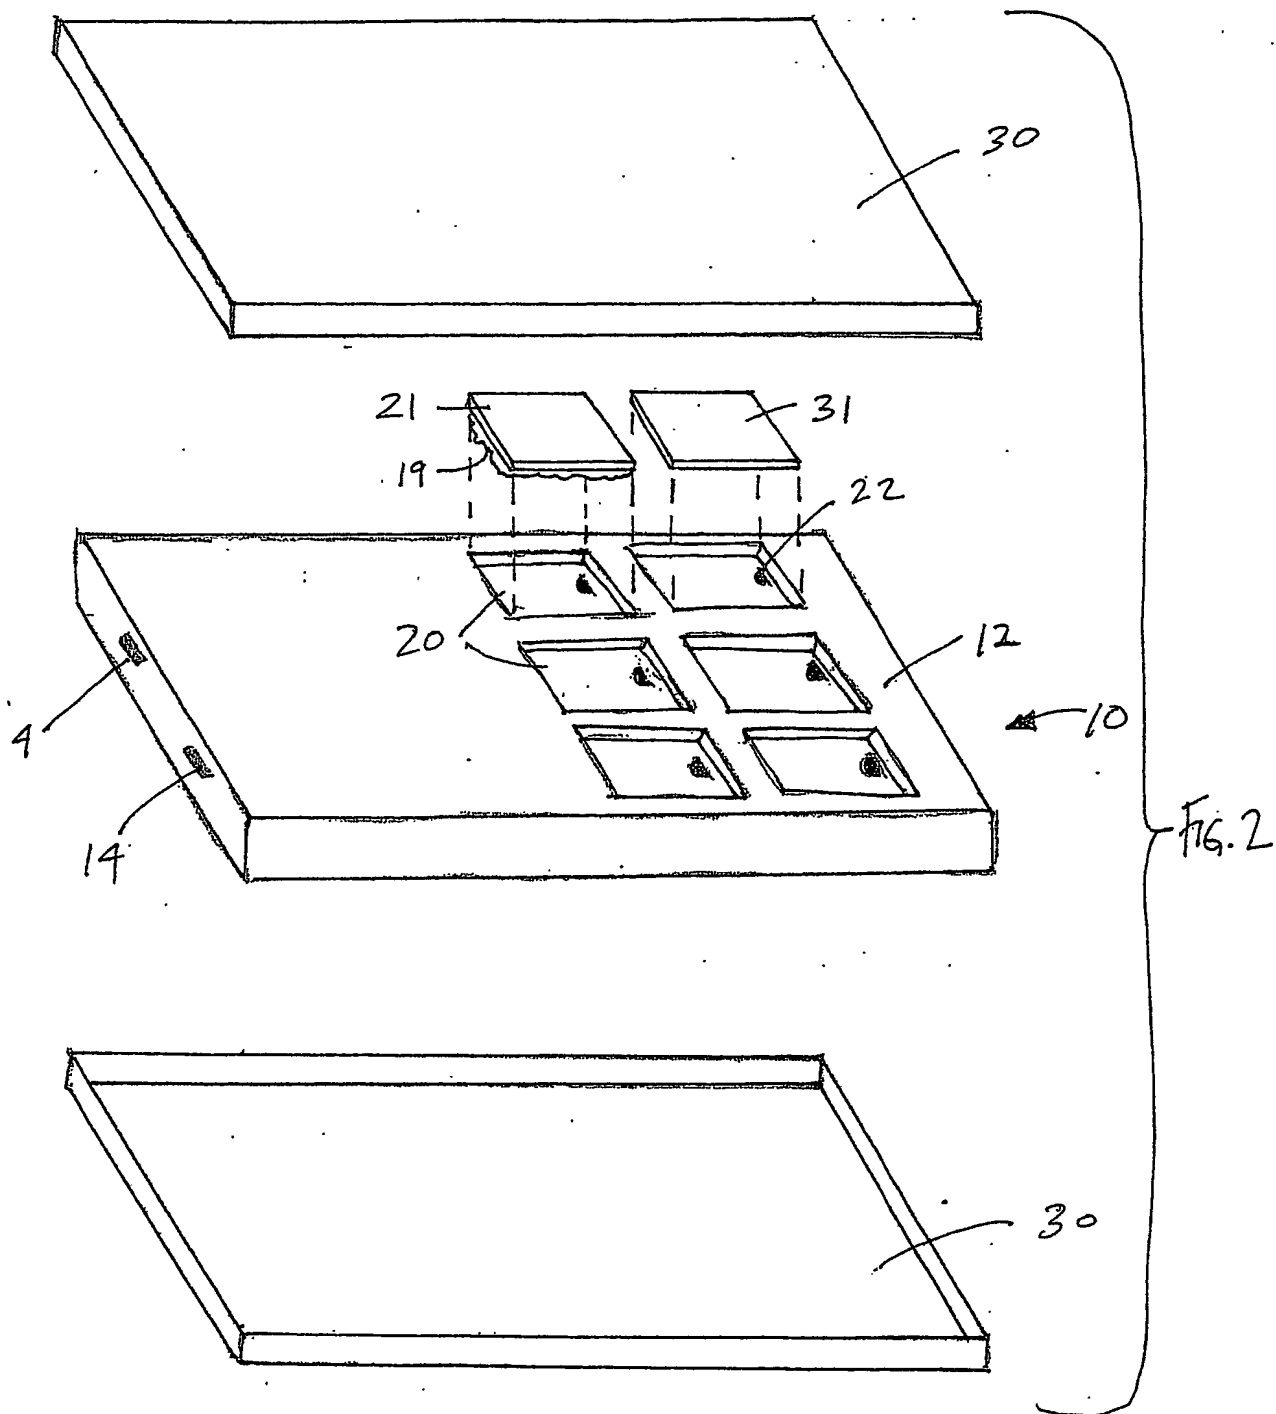

BEST AVAILABLE COPY

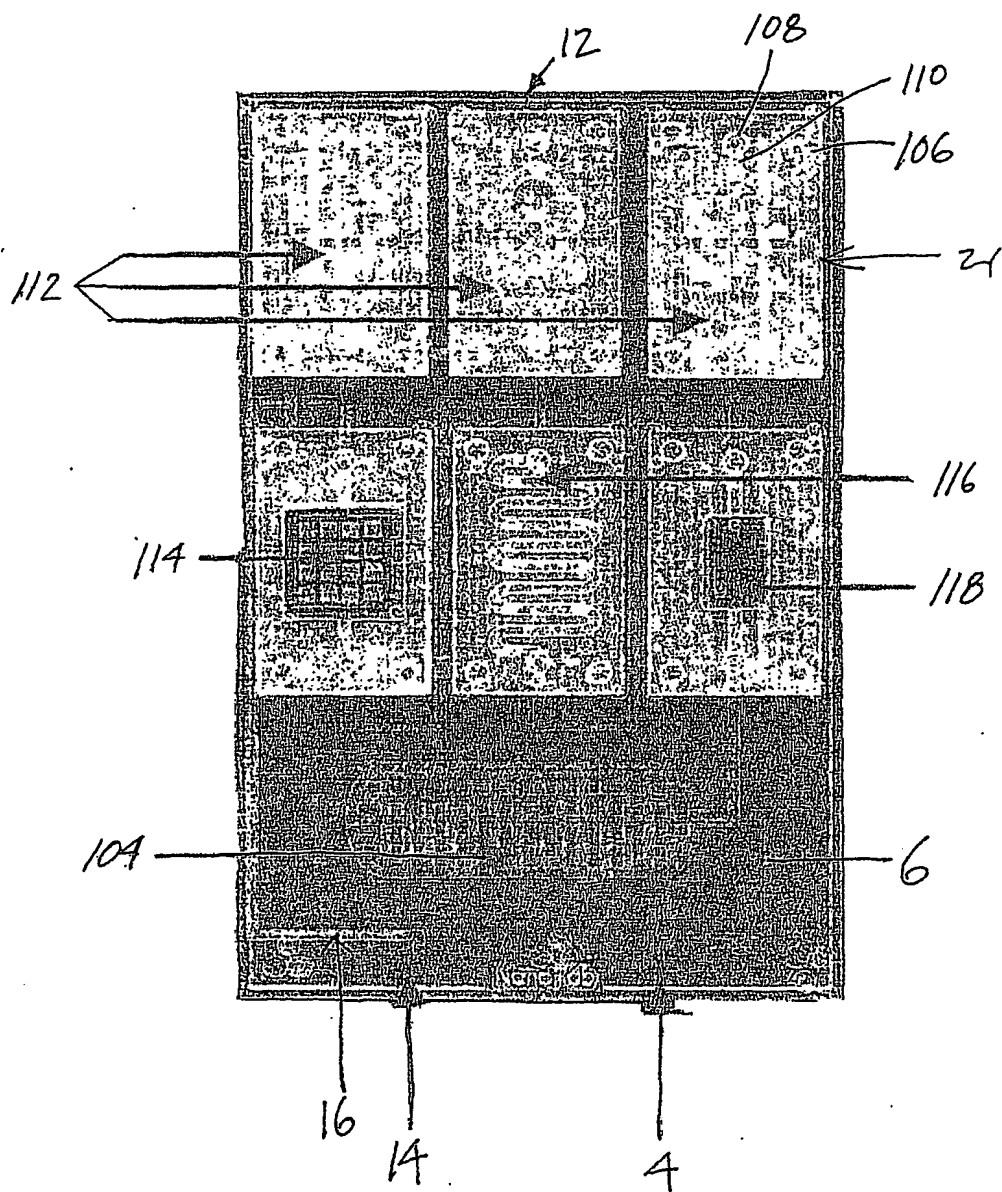


FIG. 3




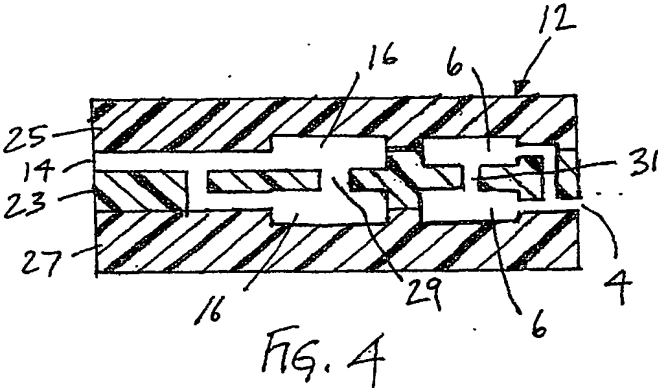


FIG. 5C












FIG. 5D

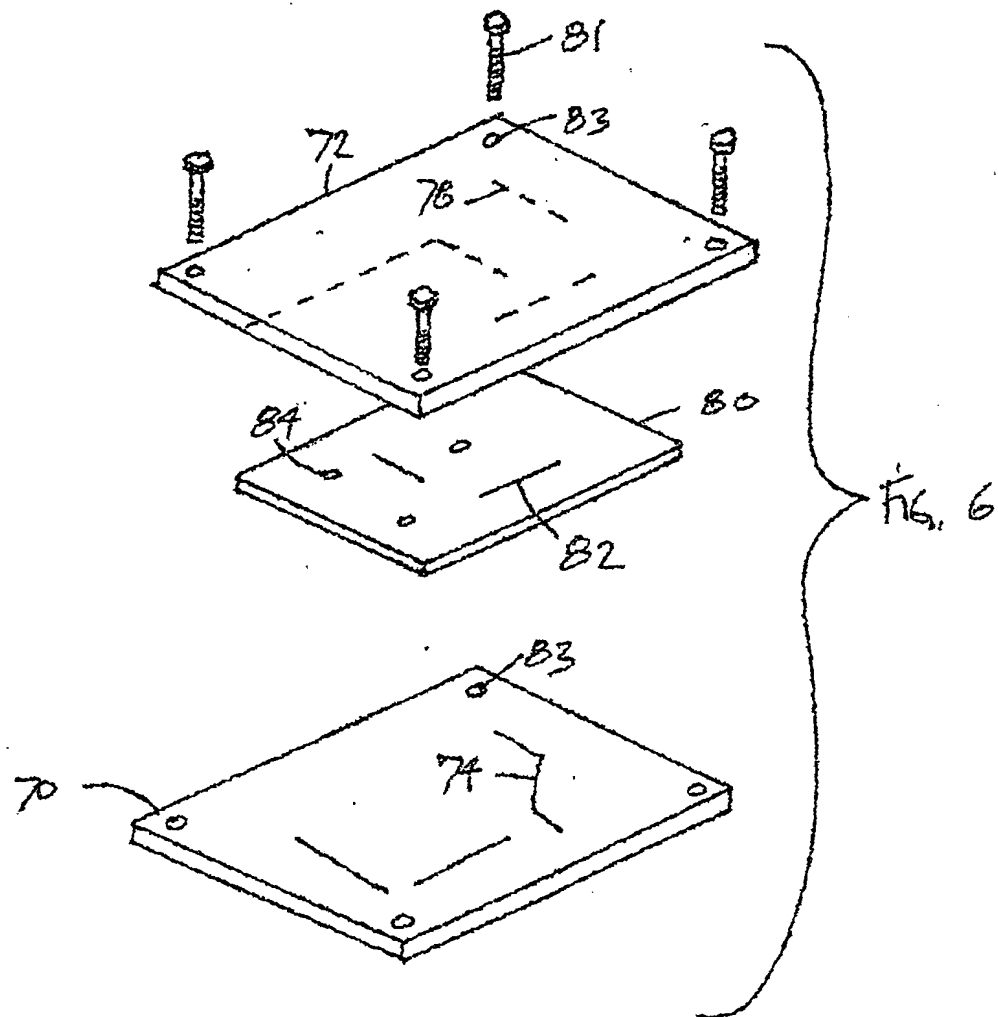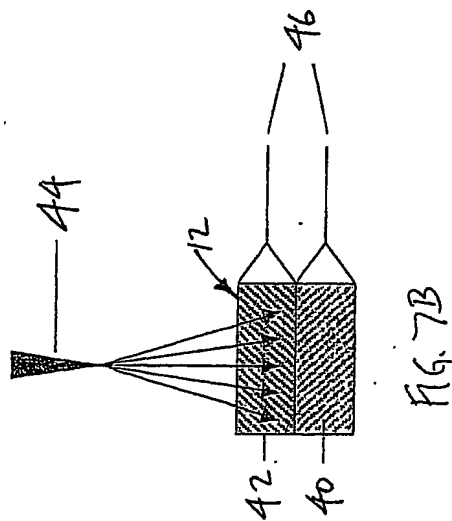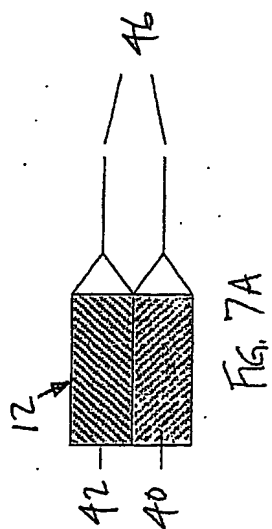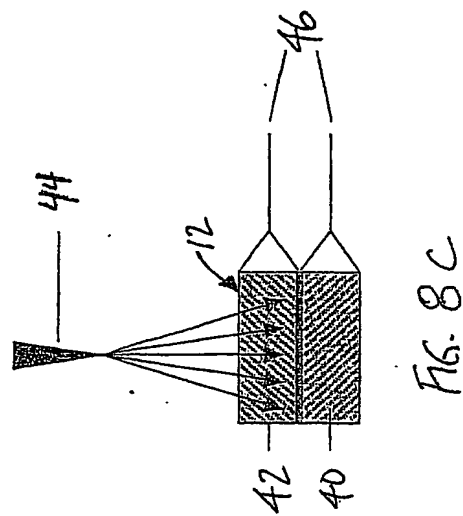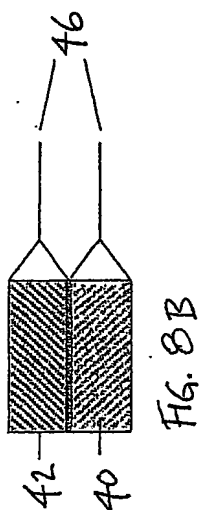


BEST AVAILABLE COPY

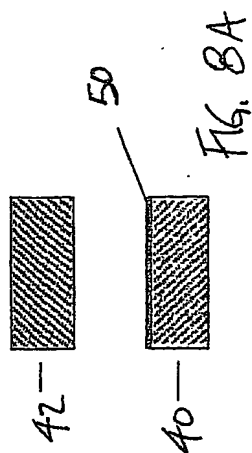

BEST AVAILABLE COPY

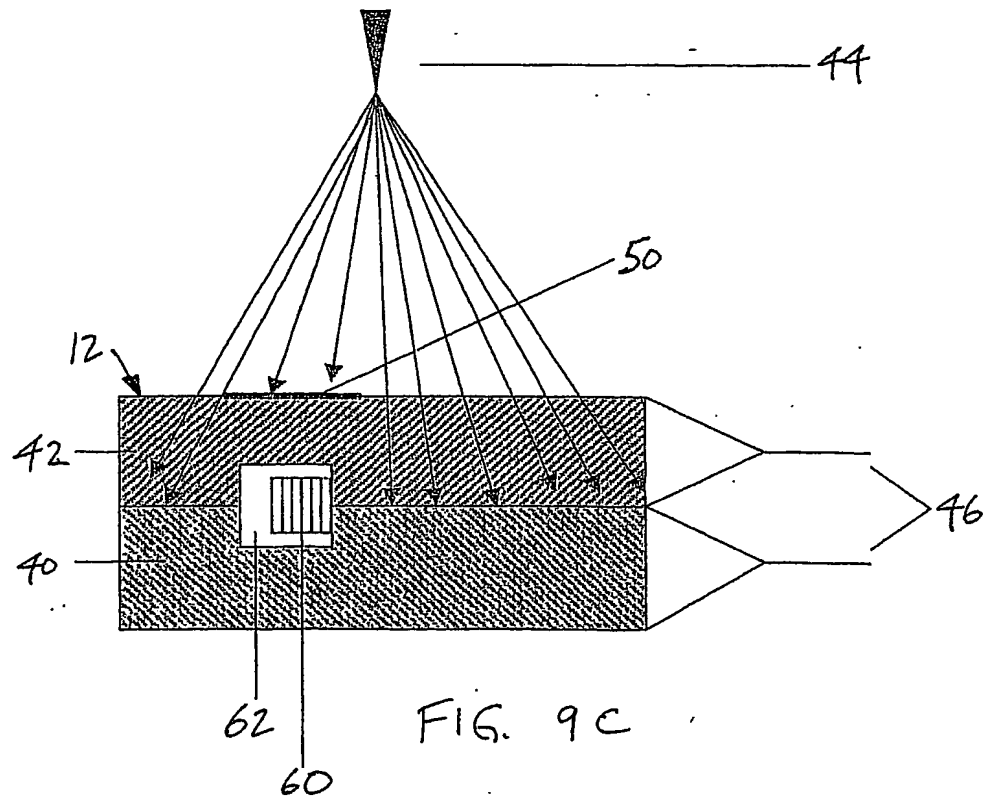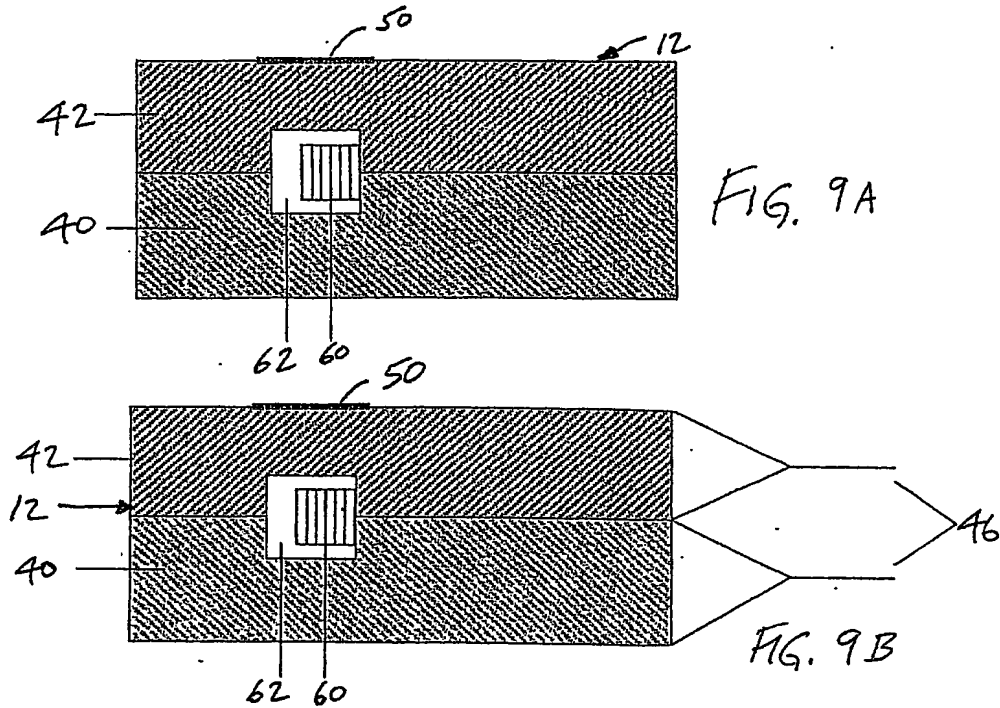



Inject Position

FIG 10B

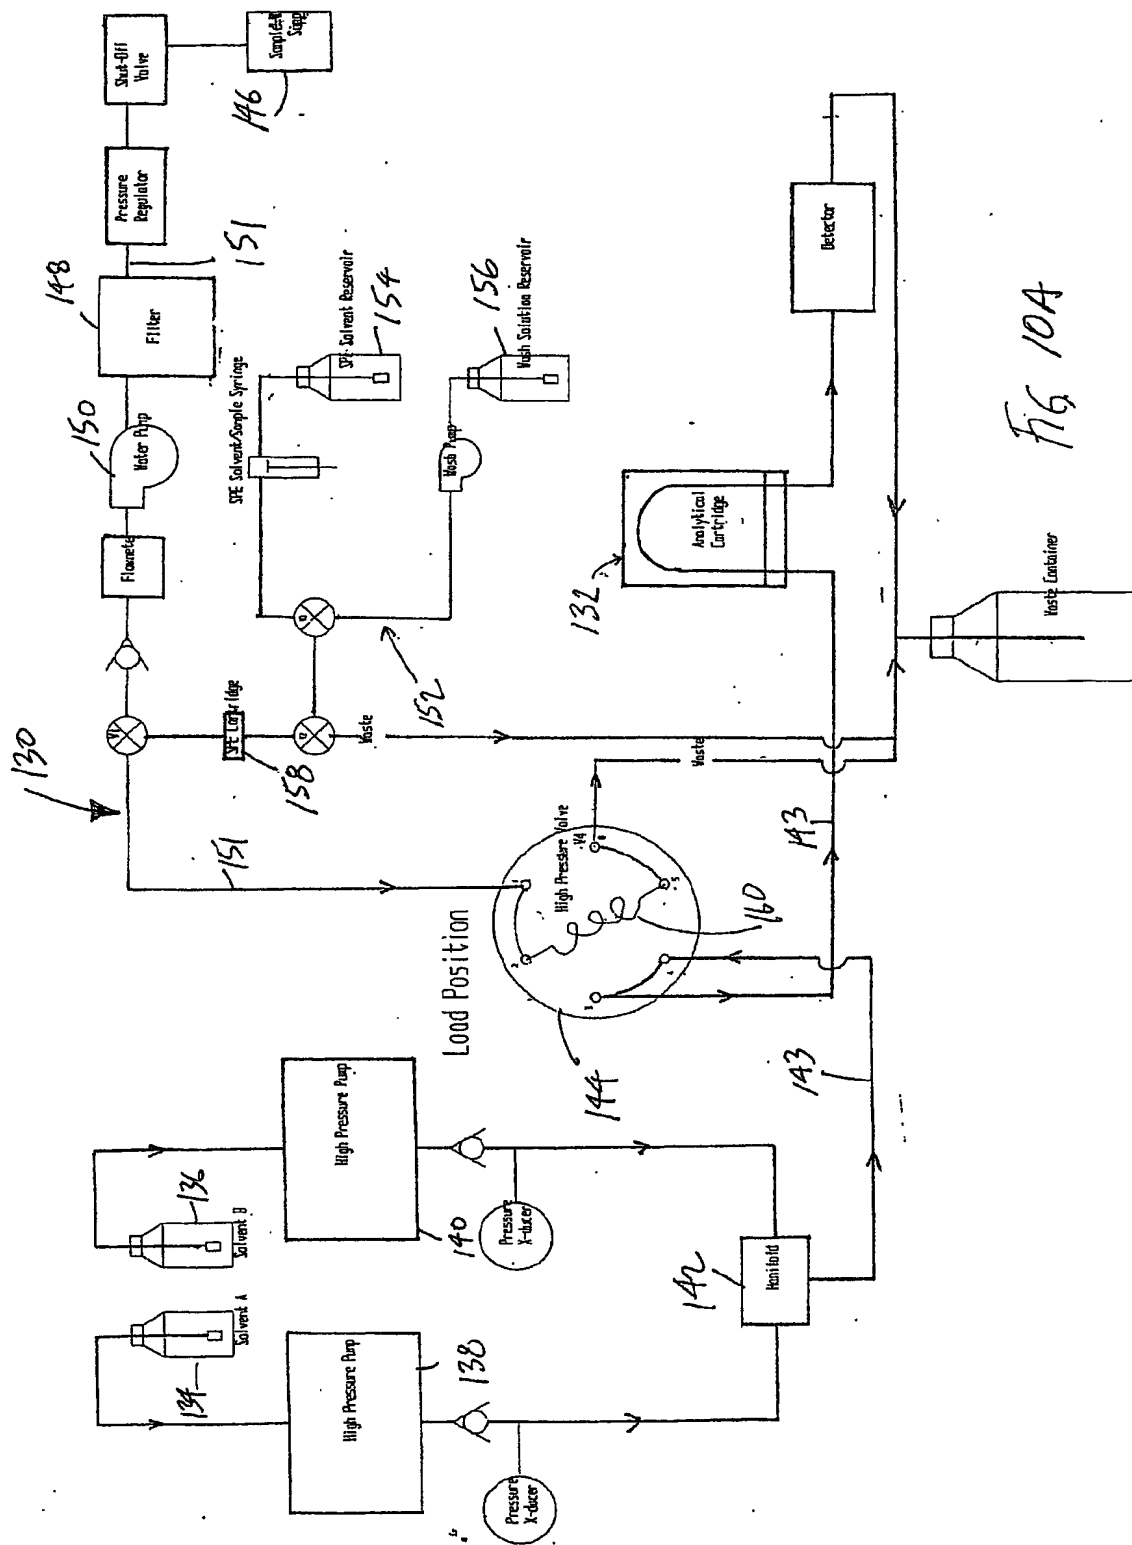


FIG 10A



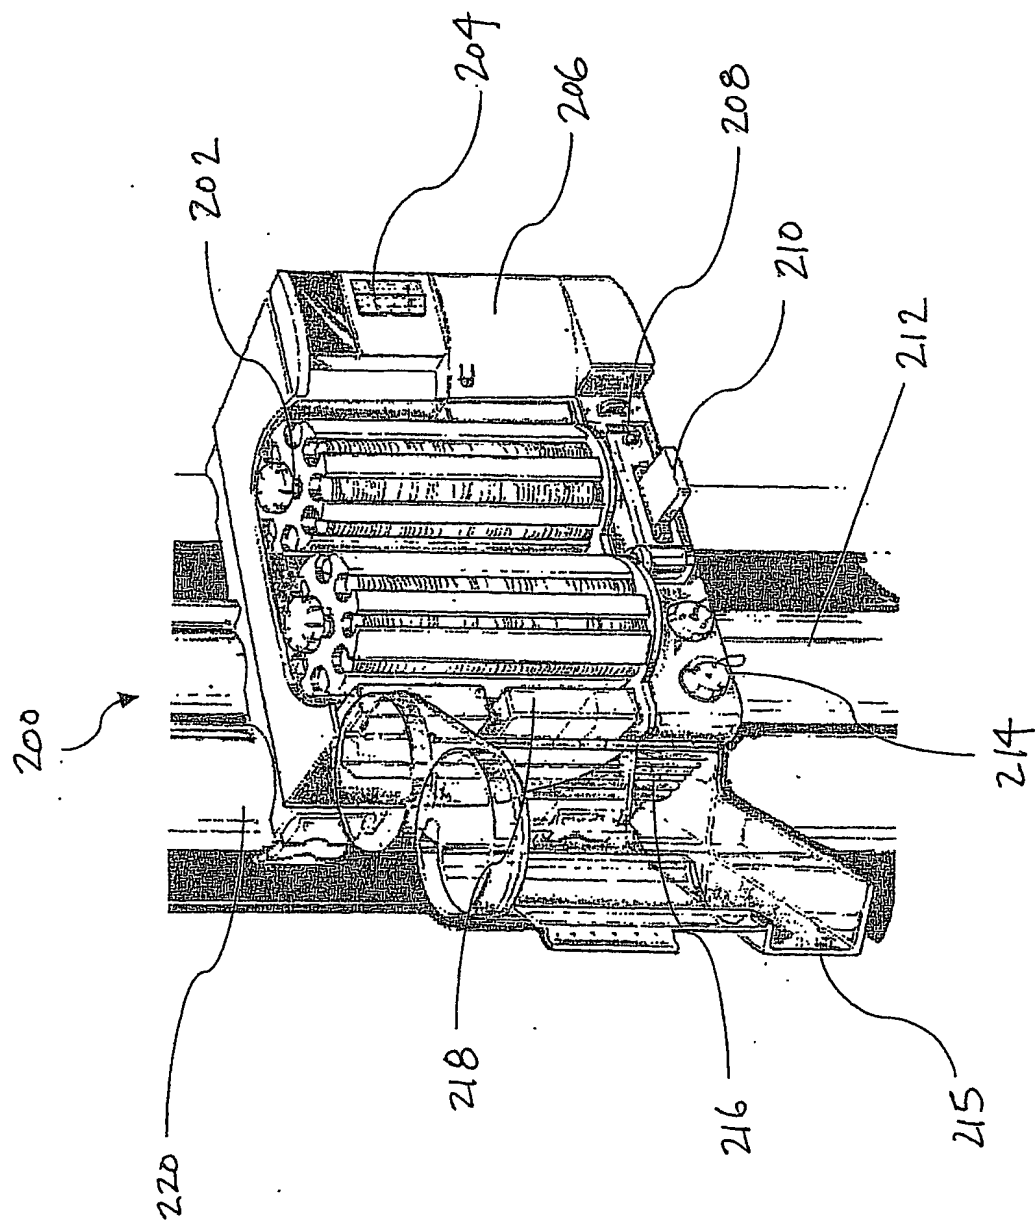


Fig. 11

BEST AVAILABLE COPY

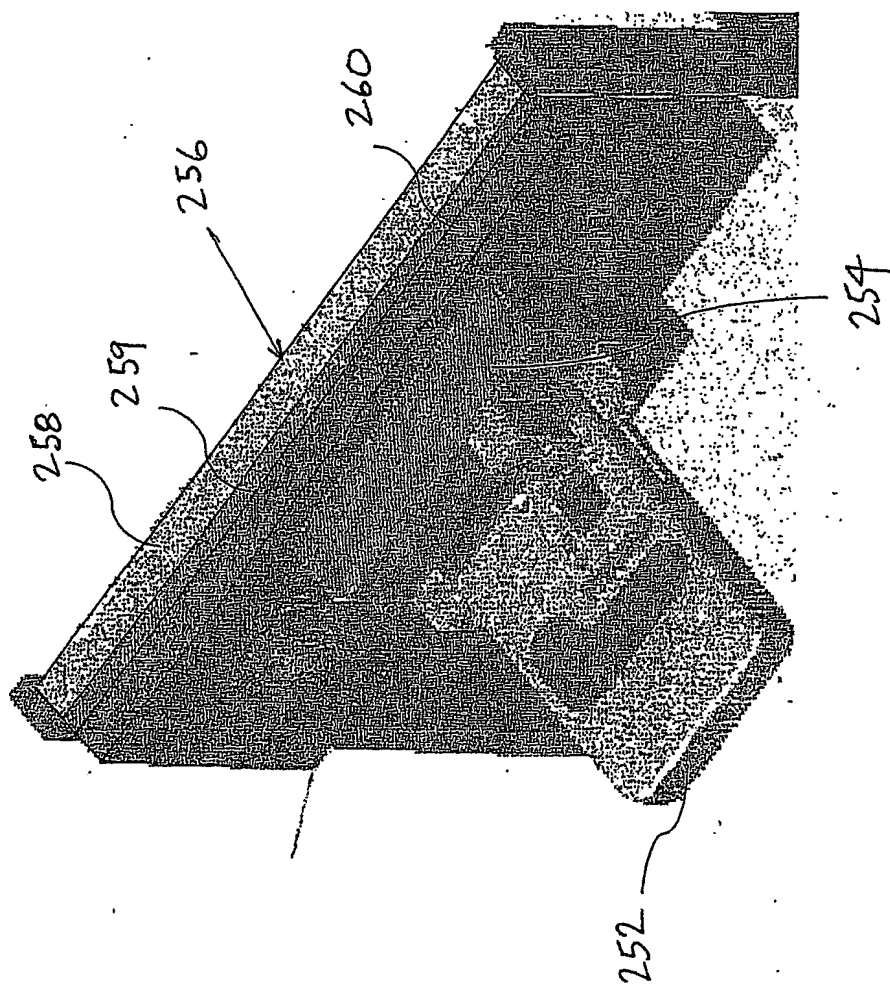


Fig. 12

BEST AVAILABLE COPY

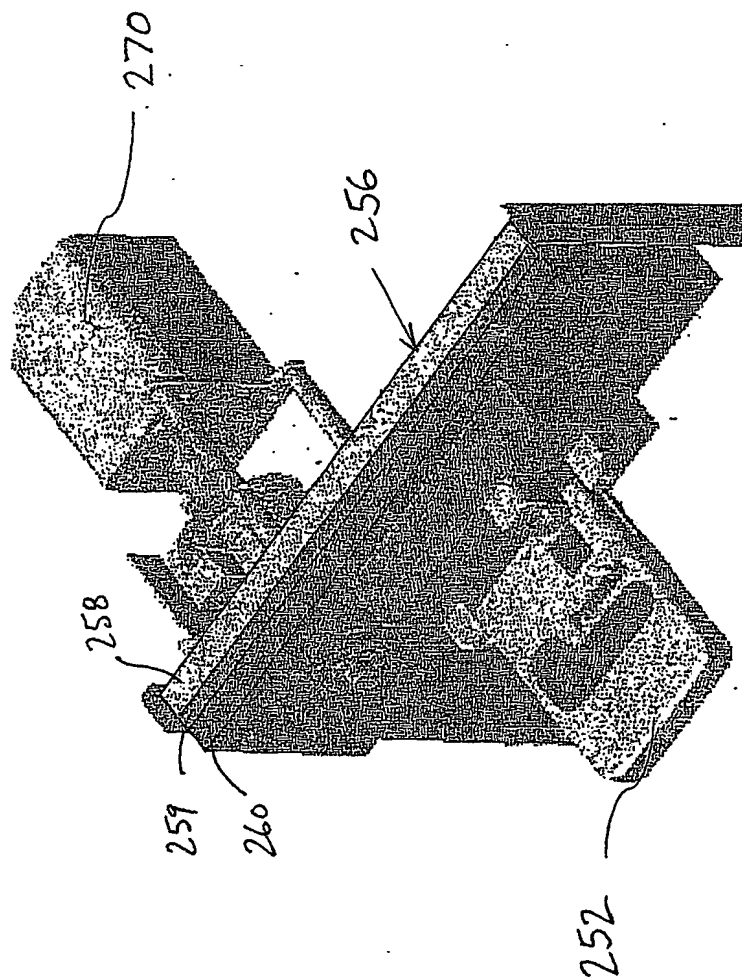


Fig. 13

BEST AVAILABLE COPY

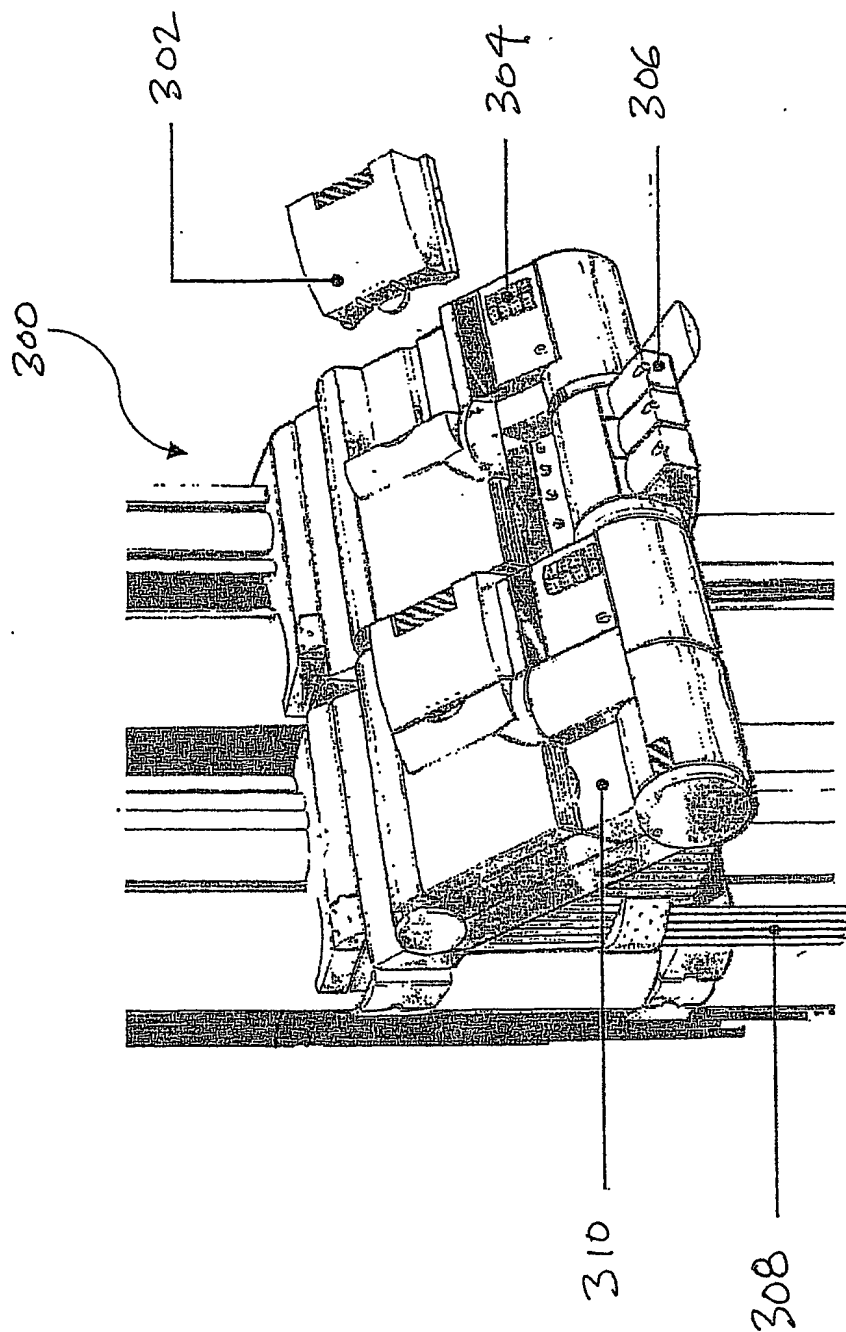


Fig. 14